



## Real-time display

Test date: 02.09.2013


## Tested equipment

<b>Generator</b>		
Name:	Model:	Type: HF/DC
Serial #:	Manufacturer:	
<b>Tube</b>		
Name:	Insert type:	Serial #:
Manufacturer:		


## Measurements

#	Tube voltage (kV)	Exposure time (ms)	Exposure (mGy)	Exposure rate (mGy/s)	HVL (mm Al)	Total filtr. (mm Al)
1	54,74	3046	5,933	1,945	2,23	3,4
2	54,44	3037	6,051	1,990	2,21	3,4
3	54,17	96,37	0,1865	1,839	2,19	3,3
4	53,02	96,35	0,1873	1,728	2,10	3,2
5						

Exposure #1




Exposure #2

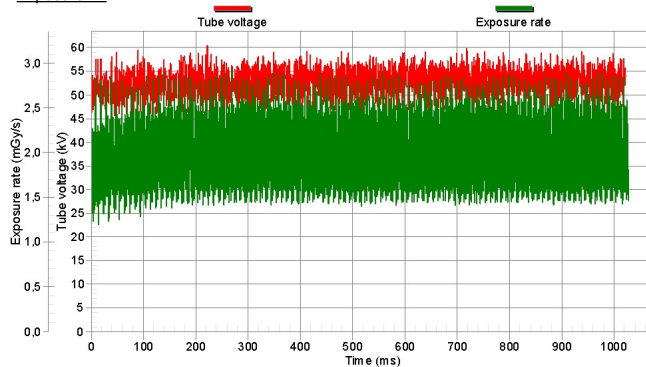




Exposure #3

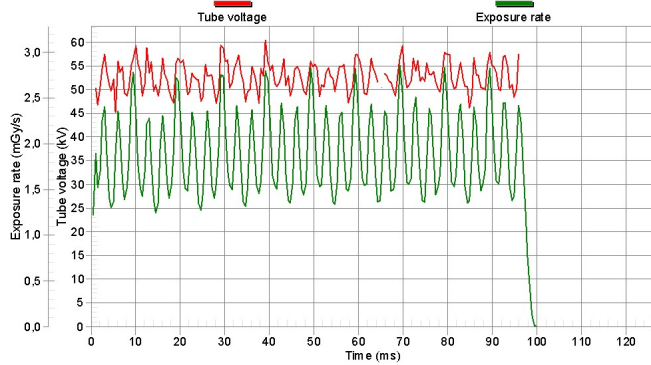

Exposure #4



## Test equipment used

Meter(s): Piranha S/N CB2-13060413  
Detector(s): MPD S/N MP2-13060415